



POLICE DEPARTMENT  
**LAKE HAVASU CITY**  
2360 McCULLOCH BOULEVARD NORTH  
LAKE HAVASU CITY, ARIZONA 86403-5947

To Whom It May Concern:

I hereby attest that Michael T. Maloy, Jr. is a Certified Intoxilyzer Quality Assurance Specialist for the Lake Havasu City Police Department.

I certify that the attached documentation of Standard Quality Assurance Procedures and/or Standard Calibration Check Procedure are full, true and correct copy of the original.

Michael Maloy Jr # 201  
Signature

STATE OF ARIZONA        )  
  ) ss  
COUNTY OF MOHAVE    )



Subscribed and sworn to before me this 17<sup>TH</sup> day of APRIL.

2024 by MICHAEL MALOY  
[Signature]

NOTARY PUBLIC  
9-17-2024

DATE

Commission expires: 3-16-2025

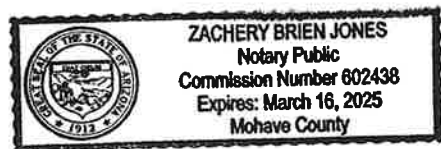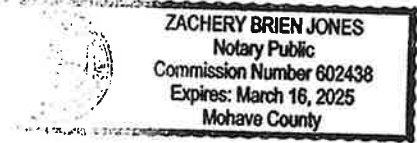

Area Code 928

Administration ..... 855-4884  
Business Office ..... 855-1171  
Investigations ..... 855-5775  
Patrol ..... 855-0515

Fax #'s  
Administration ..... 680-5430  
Business Office ..... 680-5431  
Investigations/Patrol ..... 680-5432

Emergency ..... 9-1-1  
Non-Emergency Dispatch/ ..... 855-4111  
Havasu Silent Witness ..... 854-TIPS

E-mail: police@lhcaz.gov

281

EXHIBIT I-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
INTOXILYZER MODEL 9000

PERIODIC MAINTENANCE AND STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST M. MALOY #281 AGENCY LUCPD  
DATE 04-17-2024 TIME 02:28  
INTOXILYZER SERIAL # 90-003679

1. Ensure that gas tank is attached and contains a standard alcohol concentration 0.100 AC

DIAGNOSTIC TESTS

- 1. Clock time check
- 2. Date check

OPERATIONAL TESTS

- 1. Deficient Subject Test (Proper Sample Recognition)  
Deficient Sample printed
- 2. Alcohol-free Subject Test (Proper Sample Recognition):  
0.000 AC
- 3. Mouth Alcohol Subject Test (Proper Sample Recognition):  
Invalid Sample – Begin new deprivation period printed
- 4. Radio Frequency Interference Test (Error Recognition):  
RFI Detect printed
- 5. Standard Calibration Check:  
0.101 AC
- 6. Air Blanks Completed
- 7. Timer Reset

Not a Successfully Completed Test Sequence will be printed

Instrument is operating properly and accurately. YES  NO

COMMENTS: STANDARD CHANGE P.S.I. 1,000

SIGNATURE Michael Maloy #281

281

# ARIZONA FORENSIC BREATH ALCOHOL ANALYTICAL REPORT

## INSTRUMENT INFORMATION

Analytical Instrument: Intoxilyzer 9000  
Serial Number: 90-003679  
Software Version: 9439.01.00  
Analytical Report Number: 36790417240237

QAS: MALOY, MICHAEL  
QAS Permit #: 30178  
Agency: LAKE HAVASU PD  
Last 31-Day Check: 03/29/2024  
Last Annual Maintenance: 09/22/2023

## SUBJECT INFORMATION

Name: 31-Day Check  
Test Date: 04/17/2024  
Driver's License #:  
Gender:  
Date of Birth:  
Age:

Weight:  
State of Issue:  
Driver's License Expiration:  
Deprivation Start Time: 02:00  
15 - Minute Deprivation: Yes

## OPERATOR INFORMATION

Name: MALOY, MICHAEL  
Agency: LAKE HAVASU PD

Permit #: 30178

## STANDARD INFORMATION

Standard Value: 0.100  
Standard Lot #: 302-402720275  
Expiration Date: 05/24/2025  
Bottle #: 003  
Last Changed By: MALOY, MICHAEL

Permit #: 30178

Test	g/210L	Time
Air Blank	0.000	02:28:44
Diagnostic Test	PASS	02:29:20
Air Blank	0.000	02:29:57
Calibration Chk	0.101	02:30:19
Air Blank	0.000	02:30:59
Subject Test 1	DEF*	02:34:12
Air Blank	0.000	02:35:07
Air Blank	0.000	02:35:47
Subject Test 2	0.000	02:36:25
Air Blank	0.000	02:37:07
Wait		02:41:12
Air Blank	0.000	02:41:49
Subject Test 3	INV**	02:42:34
Air Blank	RFI***	02:42:48

## RESULTS

## EXCEPTION MESSAGES

\*Deficient Sample  
\*\*Invalid Sample - Begin new deprivation period  
\*\*\*RFI Detect

\* Deficient Sample  
\*\* Invalid Sample - Begin new deprivation period  
\*\*\* RFI Detect

## OPERATOR COMMENTS

Not a Successfully Completed Test Sequence

*All air blank results must be 0.000.  
Consecutive subject test results must not differ by more than 0.020 g/210L.  
Standard check results must be ±10%.*

Intoxilyzer - Alcohol Analyzer  
Model 9000

SN: 90-003679

Test Date: 04/17/2024

Test Time: 02:25

Location:

Software Version: 9439.01.00

Standard Lot #: 302-402720275

Standard Value: 0.100

Expiration Date: 05/24/2025

Bottle #: 003

Last Changed By: MALOY, MICHAEL

Permit #: 30178

Operator: MALOY, MICHAEL

Permit #: 30178

Agency: LAKE HAVASU PD

<u>Test</u>	<u>g/210L</u>	<u>Time</u>
Air Blank	0.000	02:25:43
Calibration Chk	0.099	02:26:04
Air Blank	0.000	02:26:44

No RFI Detected

Successfully Completed Test Sequence