



POLICE DEPARTMENT  
**LAKE HAVASU CITY**  
 2360 McCULLOCH BOULEVARD NORTH  
 LAKE HAVASU CITY, ARIZONA 86403-5947

To Whom It May Concern:

I hereby attest that Michael T. Maloy, Jr. is a Certified Intoxilyzer Quality Assurance Specialist for the Lake Havasu City Police Department.

I certify that the attached documentation of Standard Quality Assurance Procedures and/or Standard Calibration Check Procedure are full, true and correct copy of the original.

Michael Maloy Jr #281  
 Signature

STATE OF ARIZONA        )  
   ) ss  
 COUNTY OF MOHAVE     )


Subscribed and sworn to before me this 28th day of August.

2022 by MICHAEL MALOY

SHAWNA MCKNIGHT  
 NOTARY PUBLIC

August 28th 2022  
 DATE

Commission expires: MAY 4, 2025

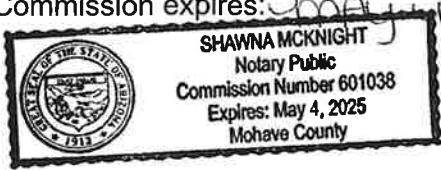

Area Code 928

- |                                |                                      |  |
|--------------------------------|--------------------------------------|--|
| Administration ..... 855-4884  | Fax #'s                              | Emergency ..... 9-1-1                  |
| Business Office ..... 855-1171 | Administration ..... 680-5430        | Non-Emergency Dispatch/ ..... 855-4111 |
| Investigations ..... 855-5775  | Business Office ..... 680-5431       | Havasu Silent Witness ..... 854-TIPS   |
| Patrol ..... 855-0515          | Investigations/Patrol ..... 680-5432 |  |

E-mail: police@lhcaz.gov

EXHIBIT I-2  
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)  
ARIZONA DEPARTMENT OF PUBLIC SAFETY  
INTOXILYZER MODEL 9000

PERIODIC MAINTENTANCE AND STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST M. MALOY #281 AGENCY LNC PD  
DATE 08-28-2022 TIME 1413  
INTOXILYZER SERIAL # 90-003680

1. Ensure that gas tank is attached and contains a standard alcohol concentration 0.100 AC

DIAGNOSTIC TESTS

- 1. Clock time check
- 2. Date check

OPERATIONAL TESTS

- 1. Deficient Subject Test (Proper Sample Recognition)  
Deficient Sample printed
- 2. Alcohol-free Subject Test (Proper Sample Recognition):  
0. 000 AC
- 3. Mouth Alcohol Subject Test (Proper Sample Recognition):  
Invalid Sample – Begin new deprivation period printed
- 4. Radio Frequency Interference Test (Error Recognition):  
RFI Detect printed
- 5. Standard Calibration Check:  
0. 094 AC
- 6. Air Blanks Completed
- 7. Timer Reset

Not a Successfully Completed Test Sequence will be printed

Instrument is operating properly and accurately. YES  NO

COMMENTS:

\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

SIGNATURE Michael Maloy #281

# ARIZONA FORENSIC BREATH ALCOHOL ANALYTICAL REPORT

## INSTRUMENT INFORMATION

Analytical Instrument: Intoxilyzer 9000  
Serial Number: 90-003680  
Software Version: 9439.01.00  
Analytical Report Number: 36800828220022

QAS: MALOY, MICHAEL  
QAS Permit #: 30178  
Agency: LAKE HAVASU PD  
Last 31-Day Check: 07/27/2022  
Last Annual Maintenance: 11/15/2021

## SUBJECT INFORMATION

Name: 31-Day Check  
Test Date: 08/28/2022  
Driver's License #:  
Gender:  
Date of Birth:  
Age:

Weight:  
State of Issue:  
Driver's License Expiration:  
Deprivation Start Time: 13:55  
15 - Minute Deprivation: Yes

## OPERATOR INFORMATION

Name: MALOY, MICHAEL  
Agency: LAKE HAVASU PD

Permit #: 30178

## STANDARD INFORMATION

Standard Value: 0.100  
Standard Lot #: 23621100A4  
Expiration Date: 11/05/2023  
Bottle #: 003  
Last Changed By: MALOY, MICHAEL

Permit #: 30178

Test	g/210L	Time
Air Blank	0.000	14:13:09
Diagnostic Test	PASS	14:13:45
Air Blank	0.000	14:14:22
Calibration Chk	0.094	14:14:44
Air Blank	0.000	14:15:23
Subject Test 1	DEF*	14:18:38
Air Blank	0.000	14:19:22
Air Blank	0.000	14:20:02
Subject Test 2	0.000	14:20:45
Air Blank	0.000	14:21:34
Wait		14:25:37
Air Blank	0.000	14:26:14
Subject Test 3	INV**	14:26:42
Air Blank	RFI***	14:26:55

## RESULTS

## EXCEPTION MESSAGES

\*Deficient Sample  
\*\*Invalid Sample - Begin new deprivation period  
\*\*\*RFI Detect

\* Deficient Sample  
\*\* Invalid Sample - Begin new deprivation period  
\*\*\* RFI Detect

## OPERATOR COMMENTS

Not a Successfully Completed Test Sequence

*All air blank results must be 0.000.  
Consecutive subject test results must not differ by more than 0.020 g/210L.  
Standard check results must be ±10%.*